LightLab 3
HS Cannabis Analyzer

Certificate of Analysis

Date:	2025-06-19 18:24:41 -04:00	Cultivar:	GLITTER BOMB
Serial:	LL030539	Moisture:	0.0%
LightLab	Midwest Hemp Analytics	Col Tests Remaining:	20
Operator:	Tim Johnston	CoA Revision:	1
Sample ID:	DGW--007	Calibration Exp:	2026-05-09
Method:	LightLab HPLC	Product:	Deep Gap Wellness
Test Type:	Hemp Compliance	SKU:	Flower
Weight / Volume:	0.5 g	Batch:	DGW
Solvent:	20 ml		
Temperature:	23.9 °C		
Notes:			

Cannabinoid Profile

Analyte	%	LOQ
THC-A	28.0	0.050
Δ9-THC	0.24	0.050
Total THC	**24.8**	

ND = Not Detected; n/a = Not Analyzed; LOQ = Limit of Quantification; Total THC = (0.877 x THC-A) + Δ9-THC; Total CBD = (0.877 x CBD-A) + CBD.

Chromatogram

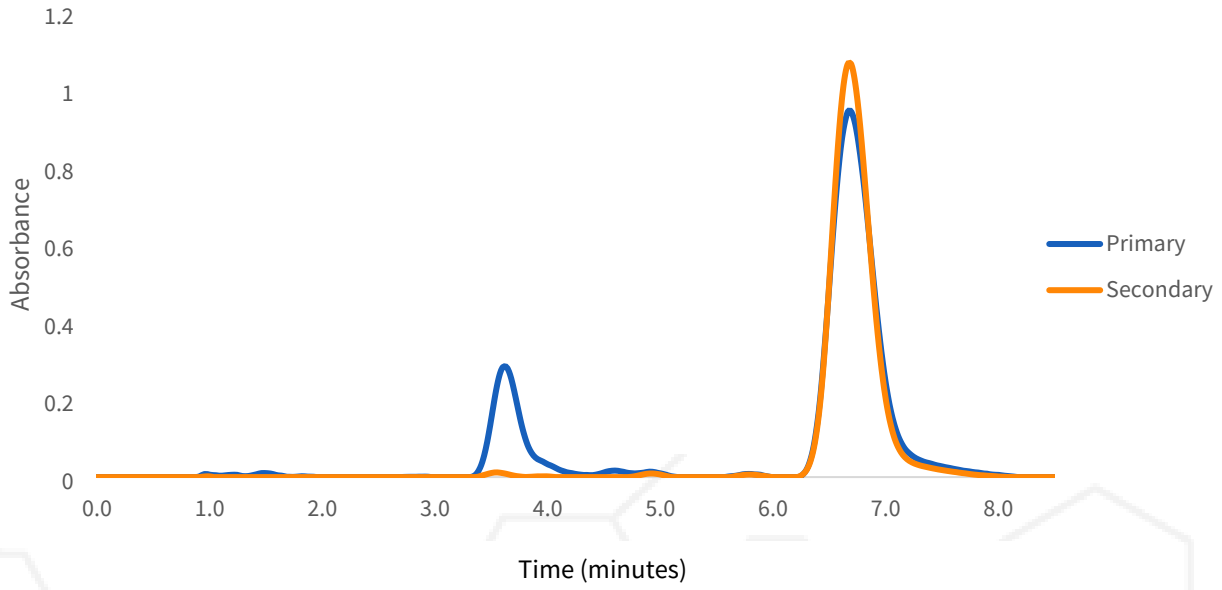

Change History

Date	User	Action
2025-06-19 18:24:41 -04:00		Test Recorded
2025-06-19 18:44:04 -04:00		Generated a CoA (revision 0)
2025-06-19 21:29:27 -04:00	TJ	Changed Operator from "MIDWEST HEMP ANALYTICS" to "Midwest Hemp Annalytics". Changed EdblProduct from "" to "Deep Gap Wellness ". Changed EdblName from "" to "Tim Johnston ". Changed Batch from "" to "DGW".
2025-06-19 21:29:55 -04:00	TJ	Changed Operator from "Midwest Hemp Annalytics" to "Midwest Hemp Analytics"
2025-06-19 21:39:54 -04:00	TJ	Changed EdblName from "Tim Johnston " to "Flower"
2025-06-19 21:41:55 -04:00	TJ	Changed SampleId from "MHA--007" to "DGW--007"
2025-06-19 21:59:22 -04:00	TJ	Changed Operator from "Midwest Hemp Analytics" to "Tim Johnston"
2025-06-19 21:59:33 -04:00		Generated a CoA (revision 1)

Scan for Authenticity

Approved Tim Johnston Date 6-19-2025

The signatory confirms that the Operator has performed the sample preparation according to the LightLab User's Guide. This report is for quality assurance purposes only. These results relate only to the sample included on this report. Orange Photonics makes no claims as to the efficacy, safety, or risks associated with any detected or non-detected level of any compounds reported herein. Orange Photonics makes no claims regarding the adherence to sample preparation guidelines, by the operator, as outlined in the LightLab User's Guide.